


# Standards for Cluster System

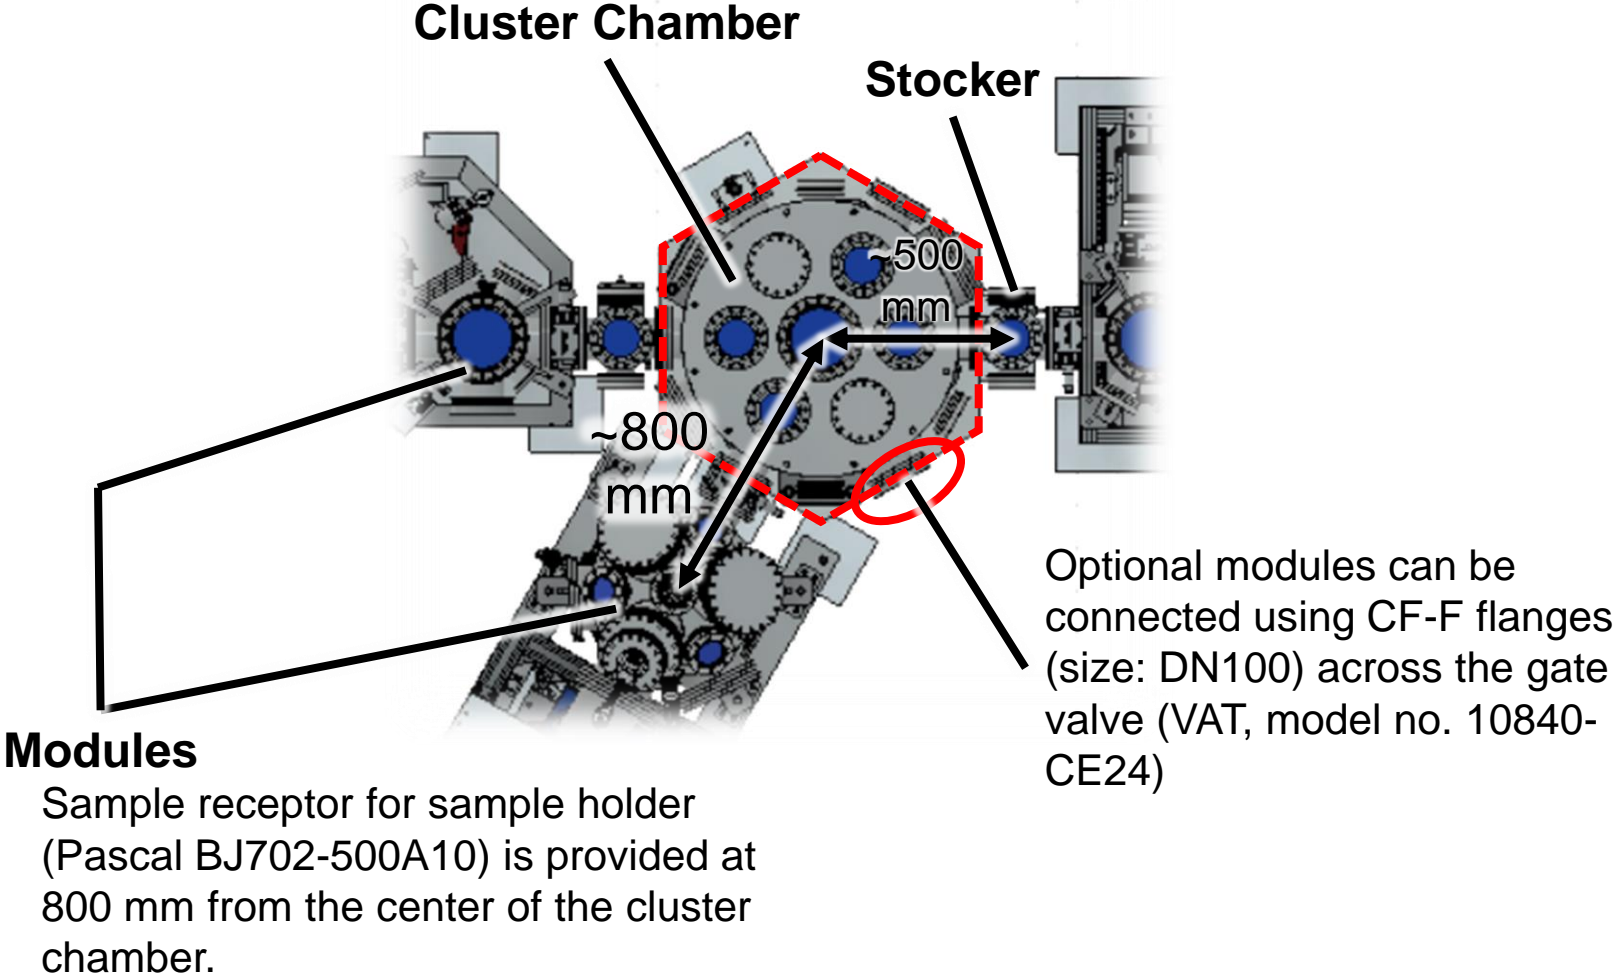

## Modules

Sample receptor for sample holder (Pascal BJ702-500A10) is provided at 800 mm from the center of the cluster chamber.

Optional modules can be connected using CF-F flanges (size: DN100) across the gate valve (VAT, model no. 10840-CE24)